




Q76299
10/603,927 Filed: 6/26/03
Darryl Mexic (202) 293-7060
Toshiaki MIZUNO, et al.
DRAINING DEVICE AND LENS PROCESSING
SYSTEM HAVING THE SAME
Page 1 of 9


FIG. 1



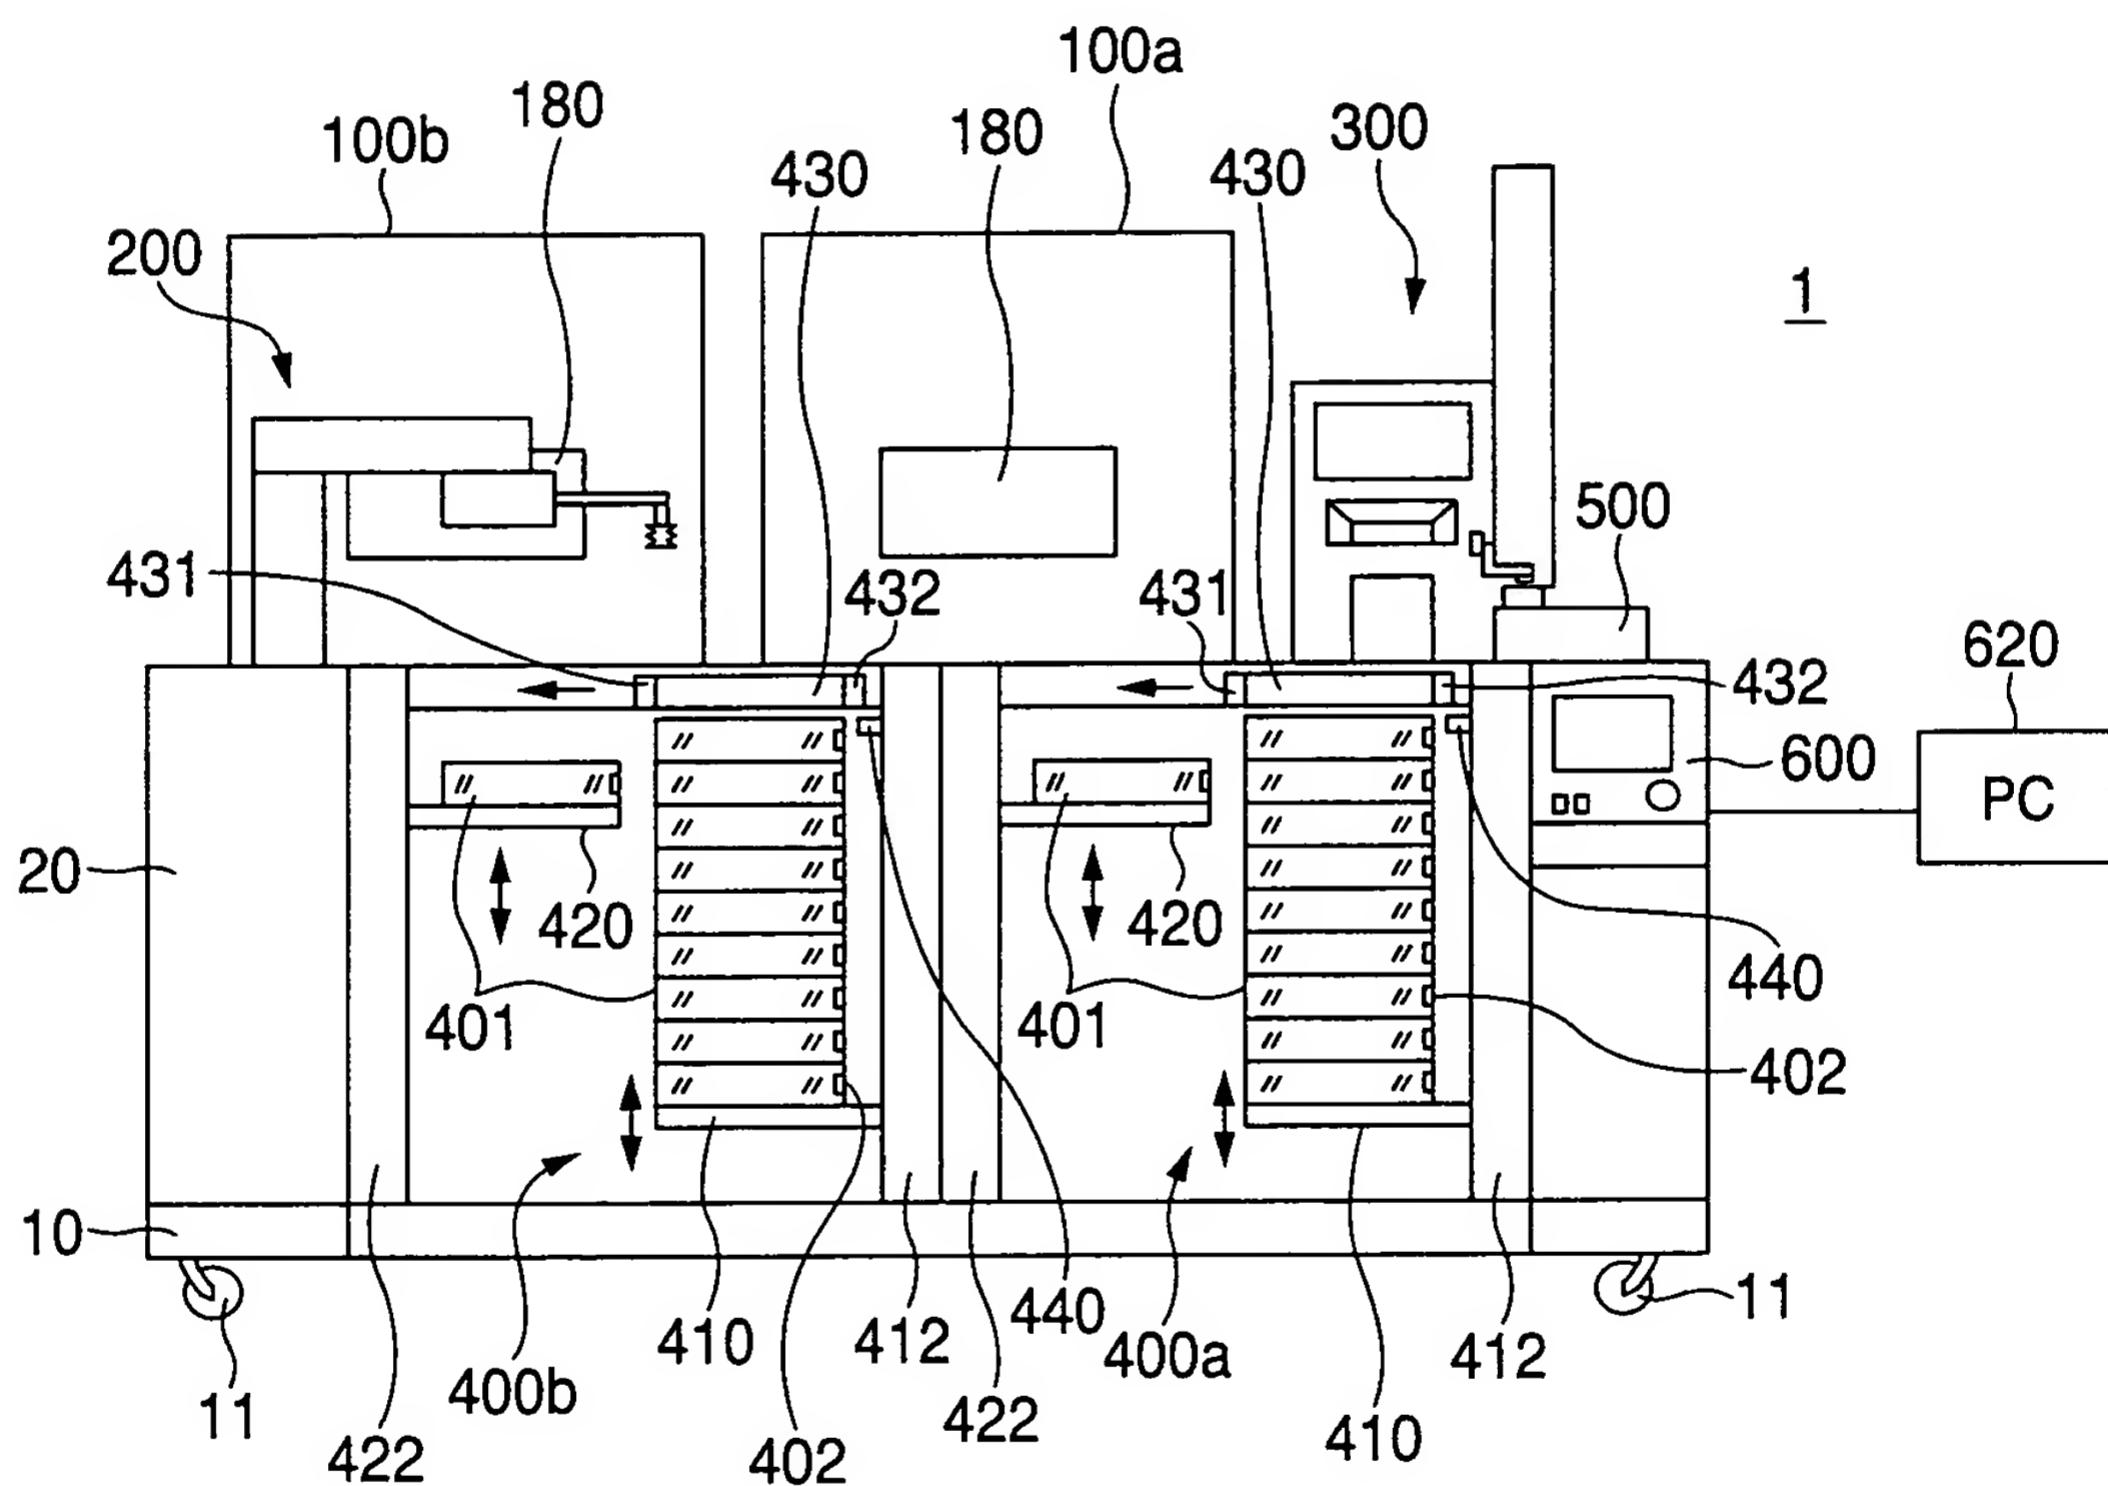

Q76299
10/603,927 Filed: 6/26/03
Darryl Mexic (202) 293-7060
Toshiaki MIZUNO, et al.
DRAINING DEVICE AND LENS PROCESSING
SYSTEM HAVING THE SAME
Page 2 of 9


FIG. 2

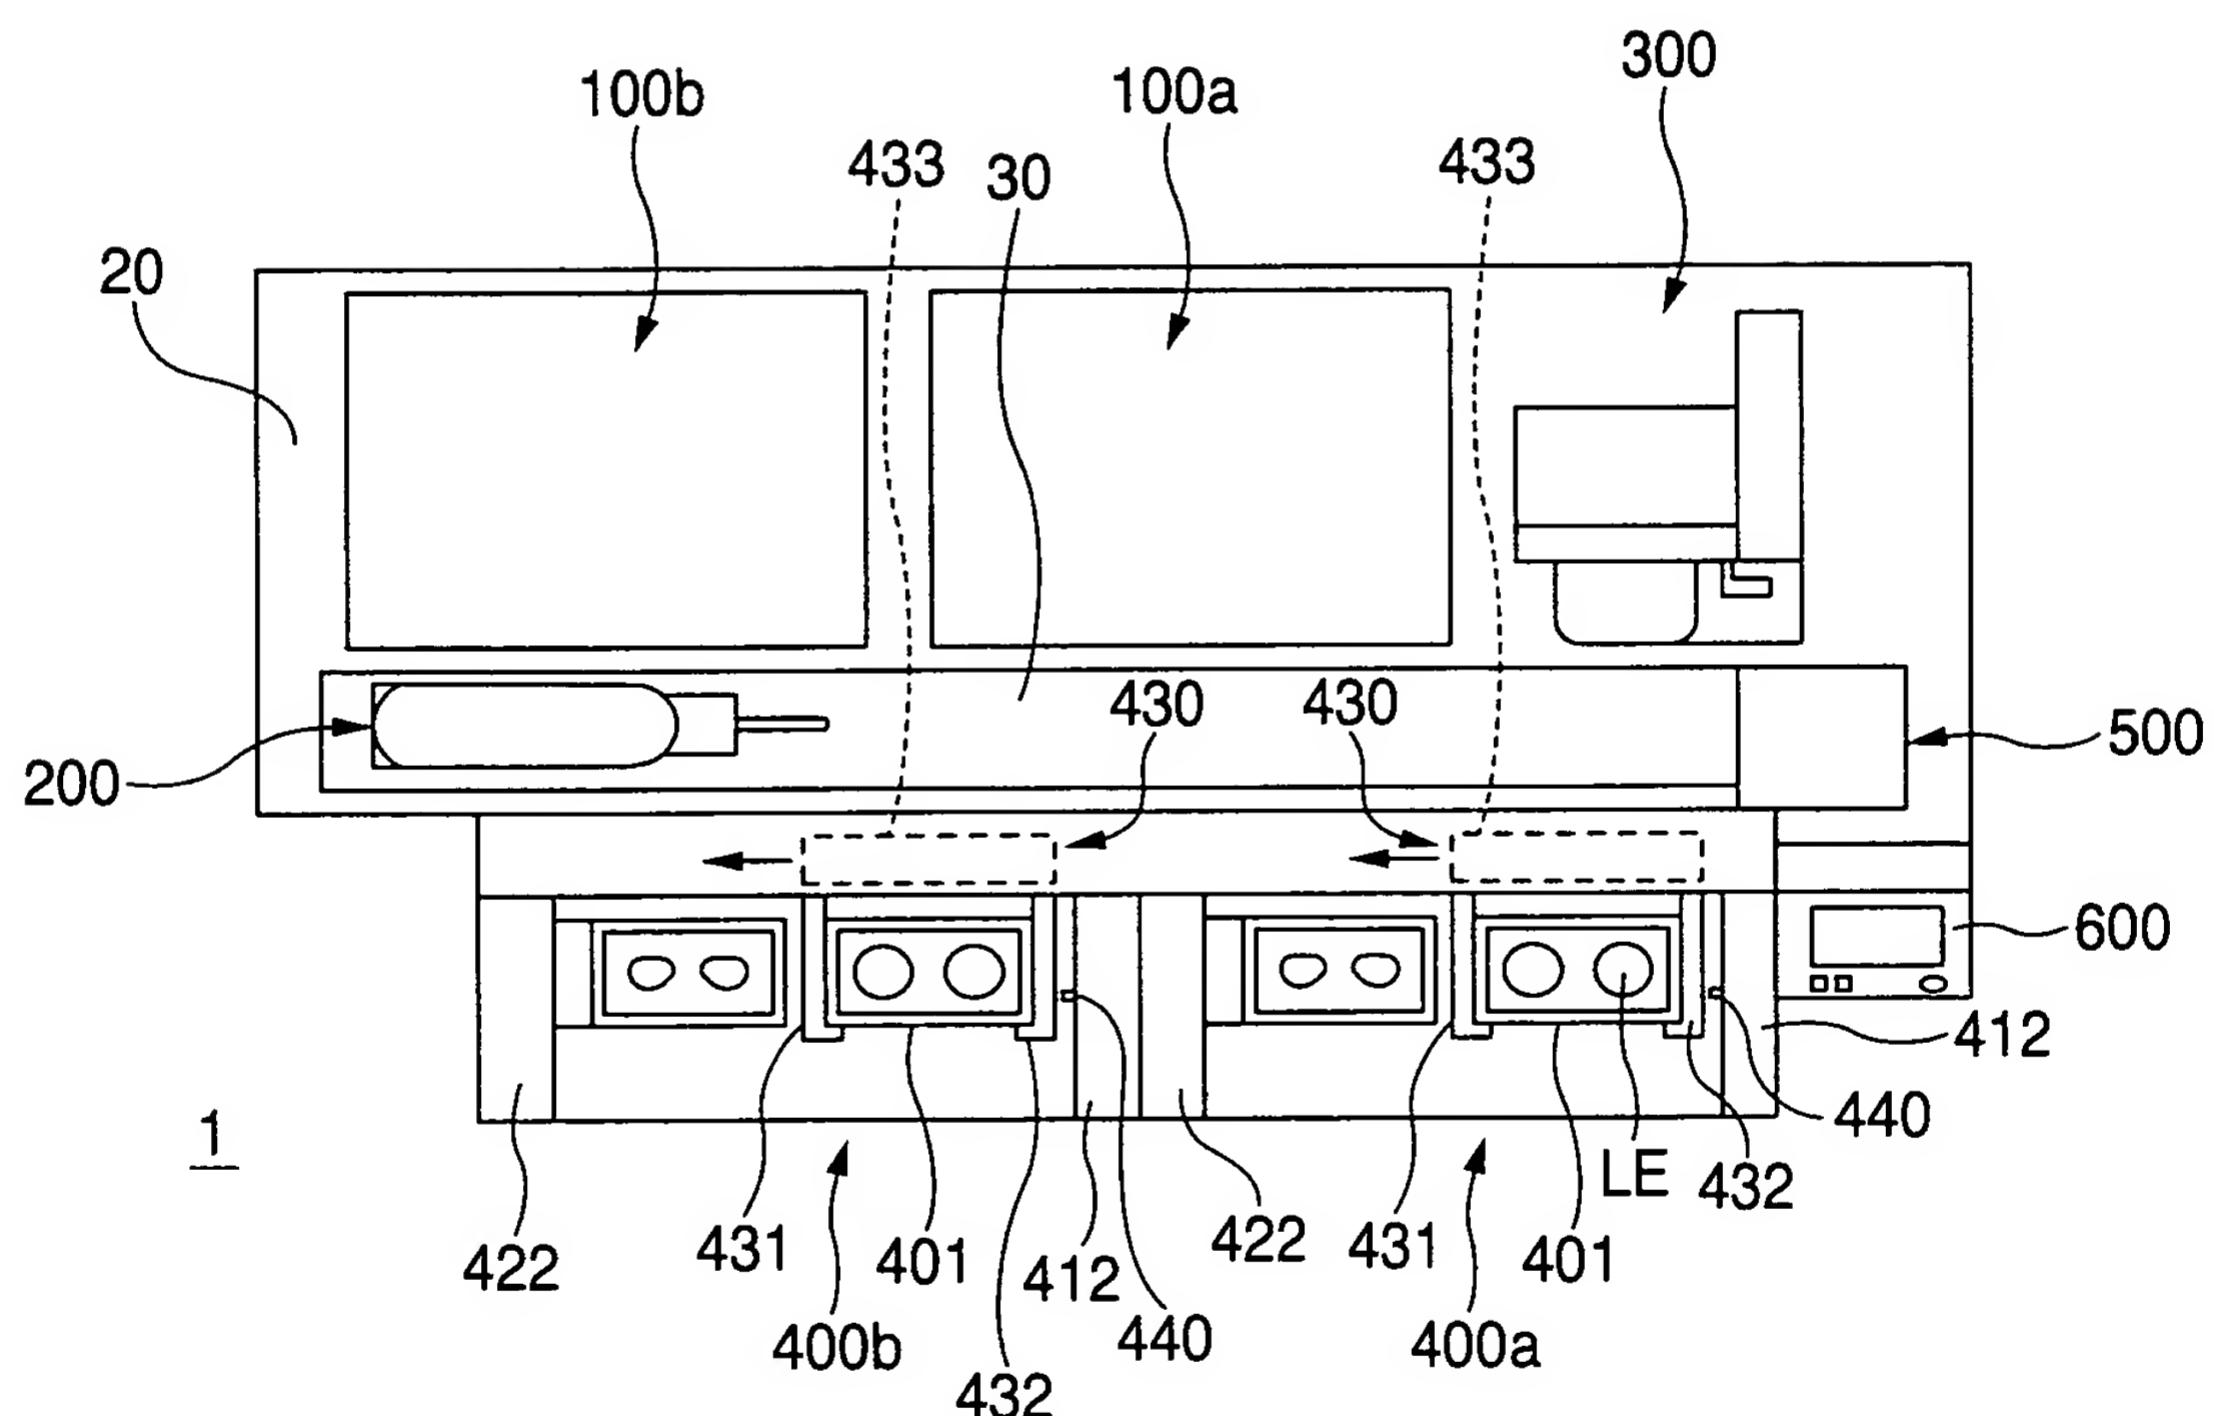



Q76299
10/603,927 Filed: 6/26/03
Darryl Mexic (202) 293-7060
Toshiaki MIZUNO, et al.
DRAINING DEVICE AND LENS PROCESSING
SYSTEM HAVING THE SAME
Page 3 of 9

FIG. 3

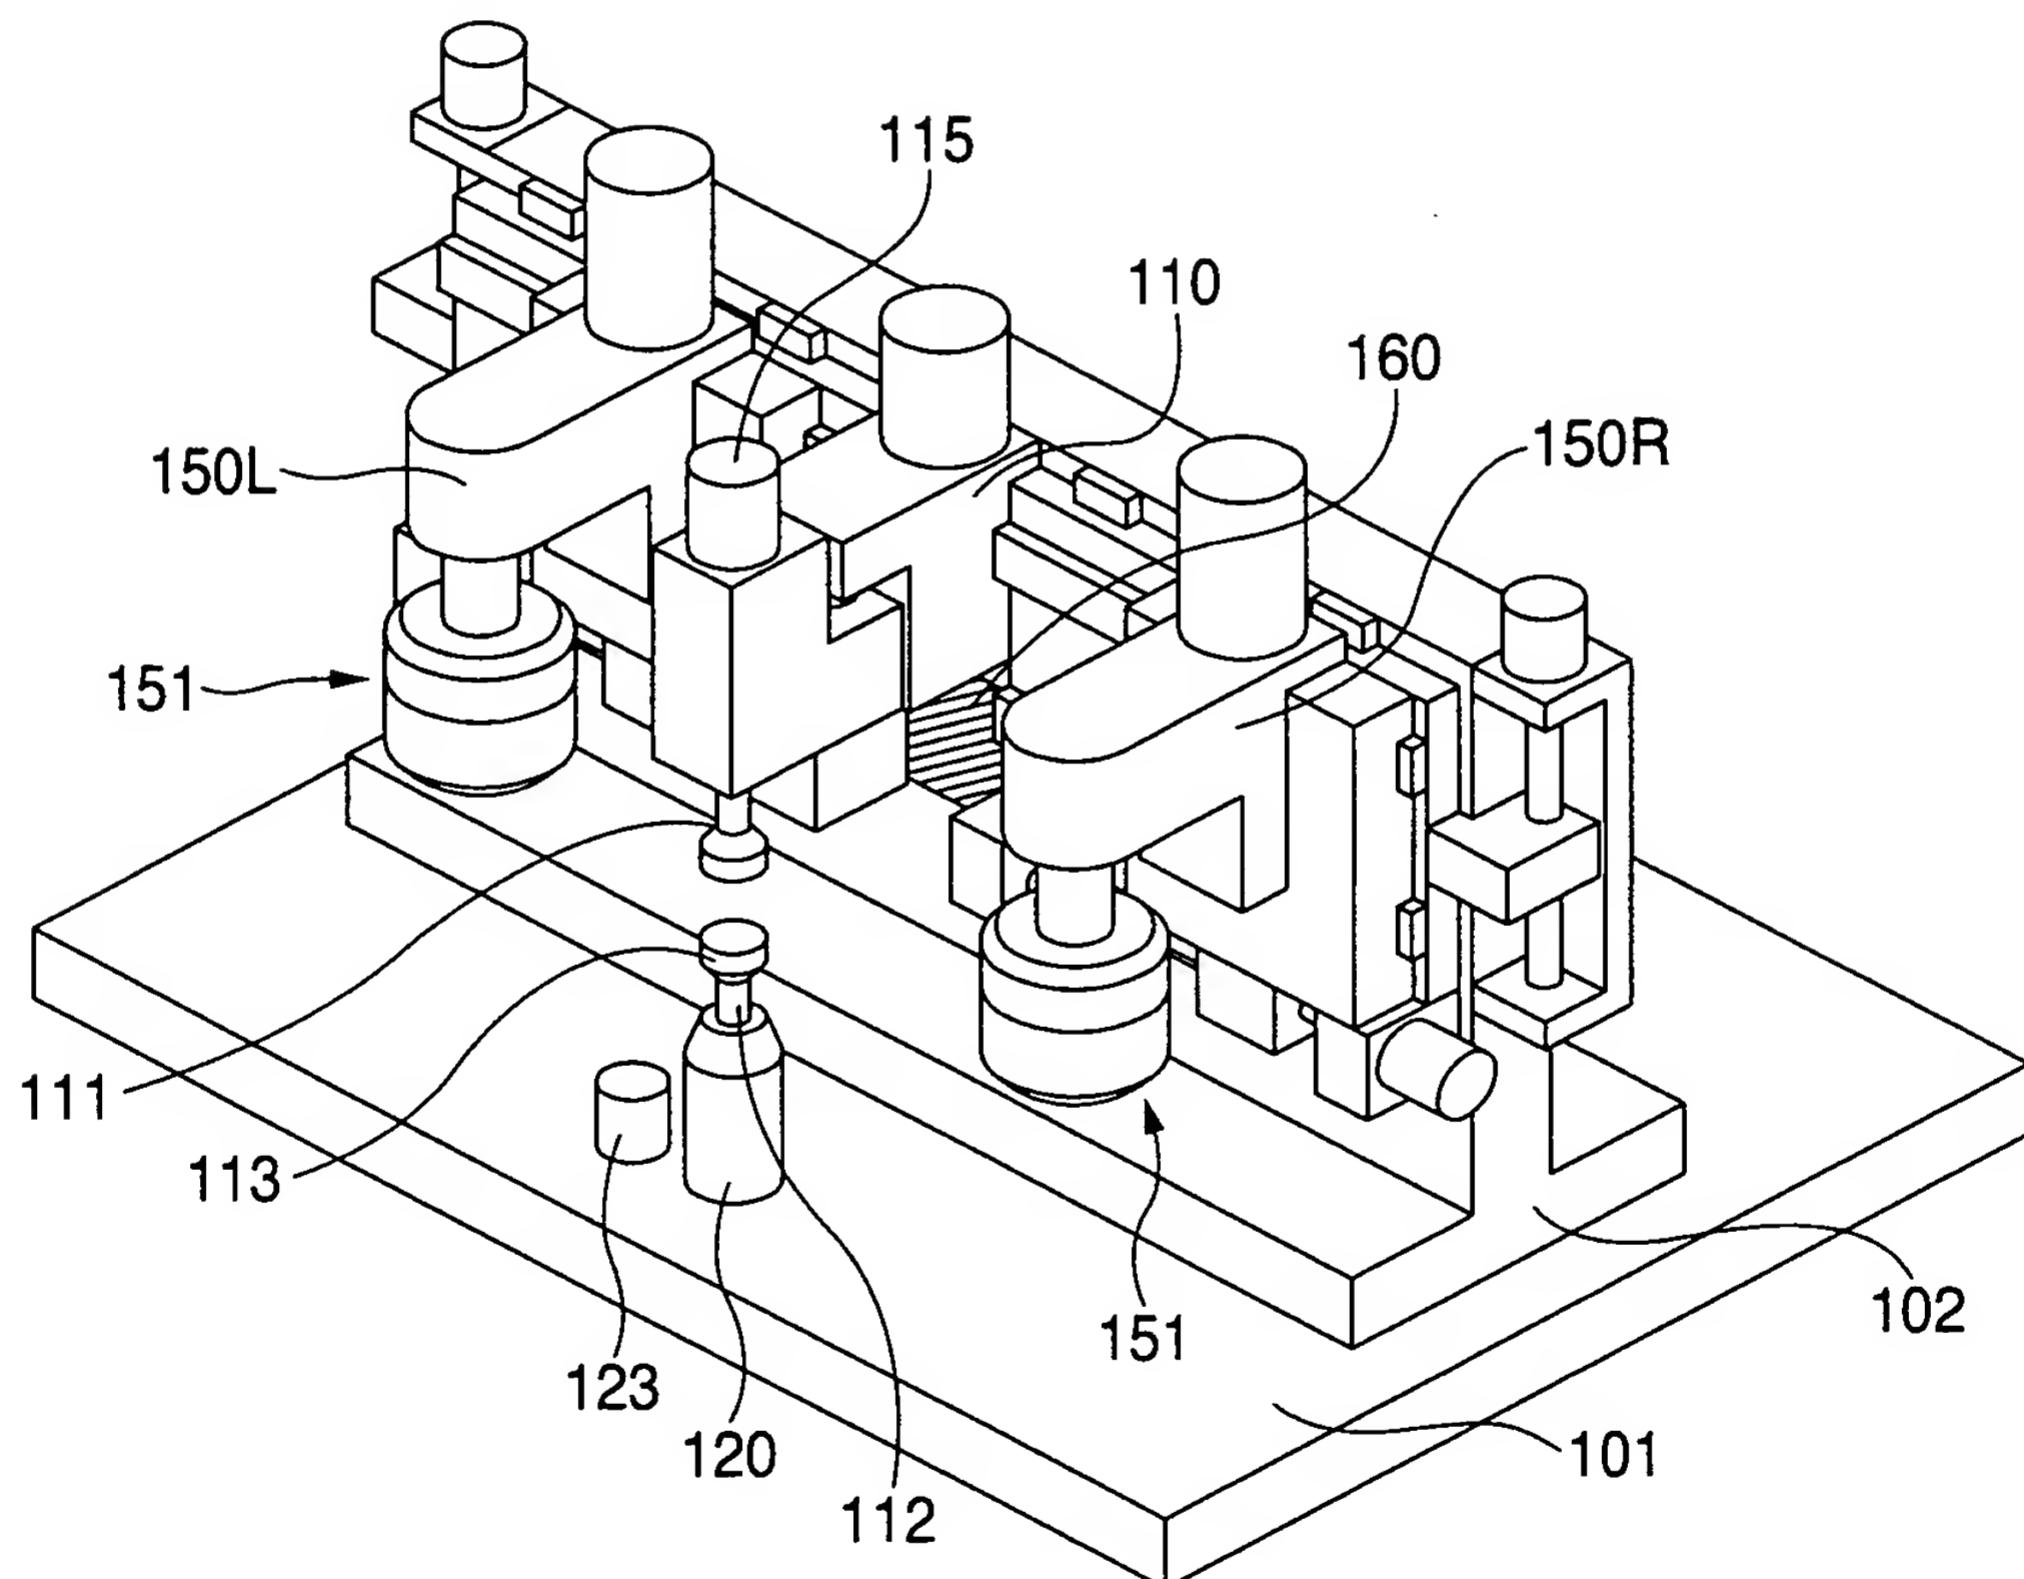



Q76299
10/603,927 Filed: 6/26/03
Darryl Mexic (202) 293-7060
Toshiaki MIZUNO, et al.
DRAINING DEVICE AND LENS PROCESSING
SYSTEM HAVING THE SAME
Page 4 of 9

FIG. 4


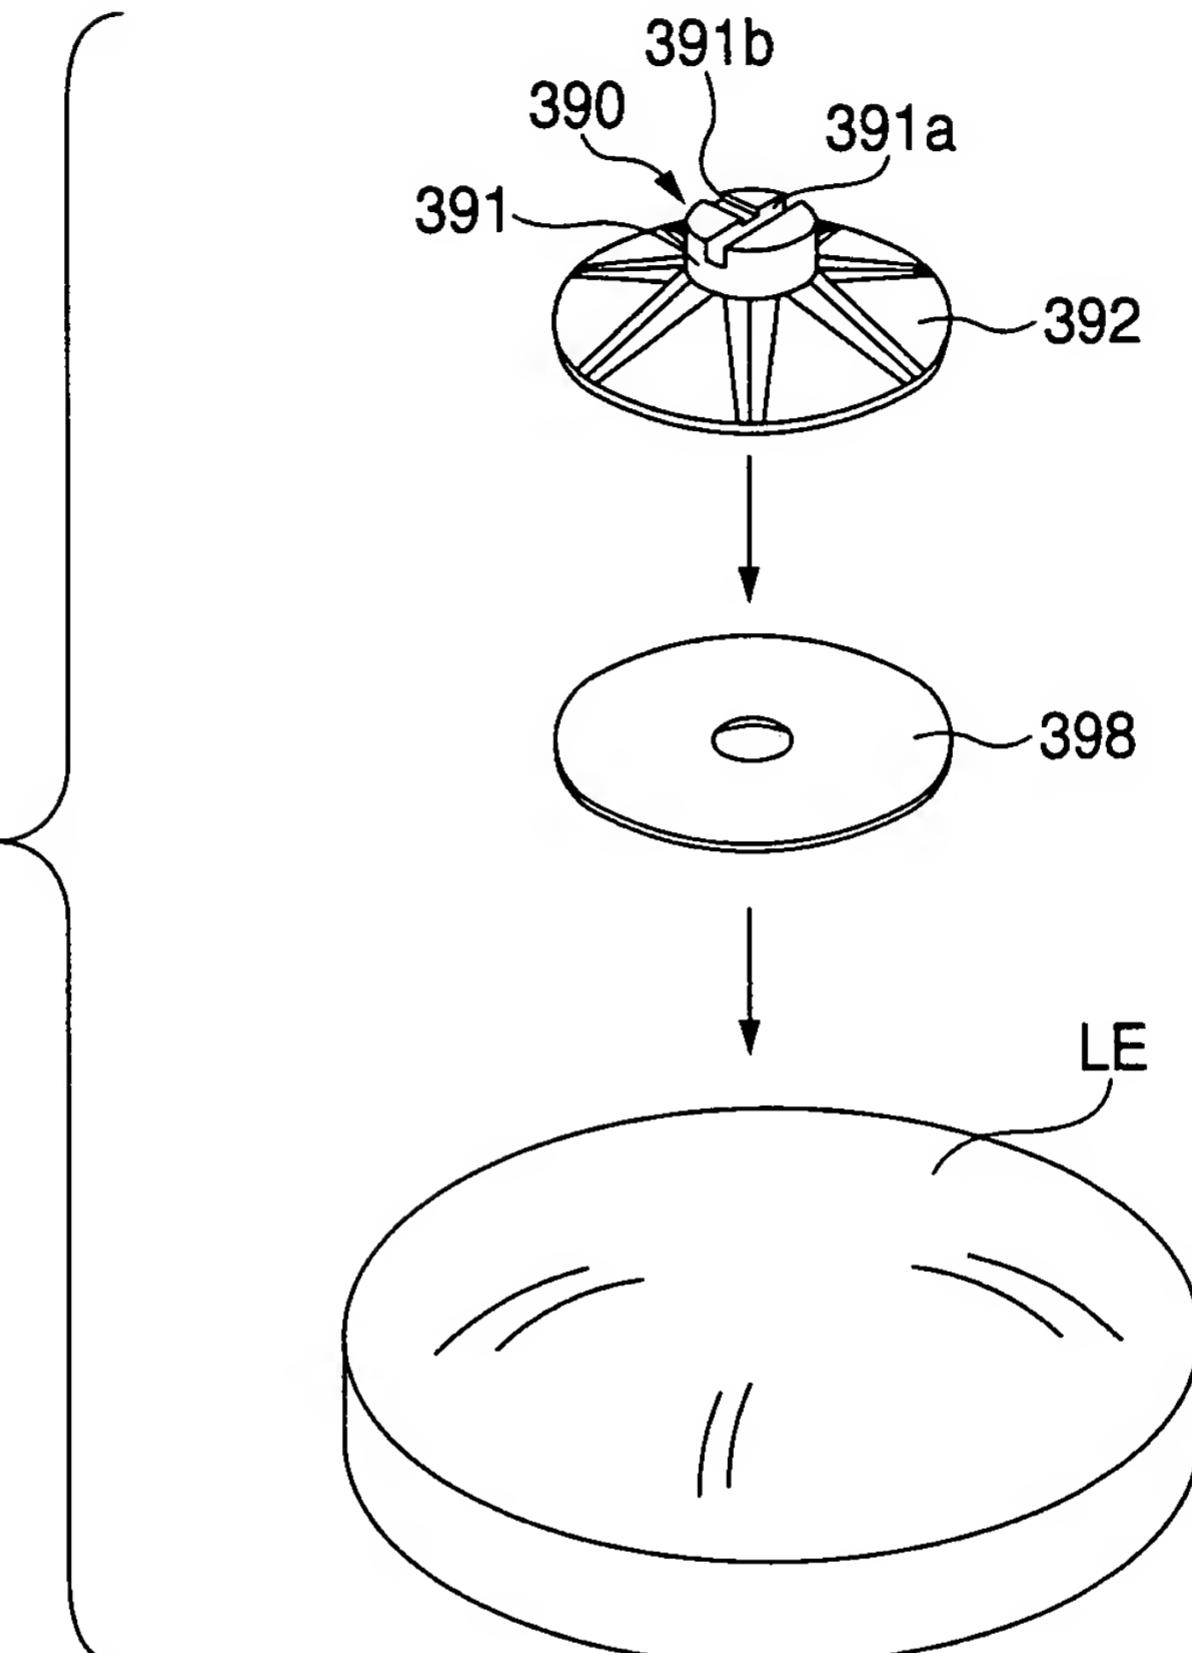


FIG. 5



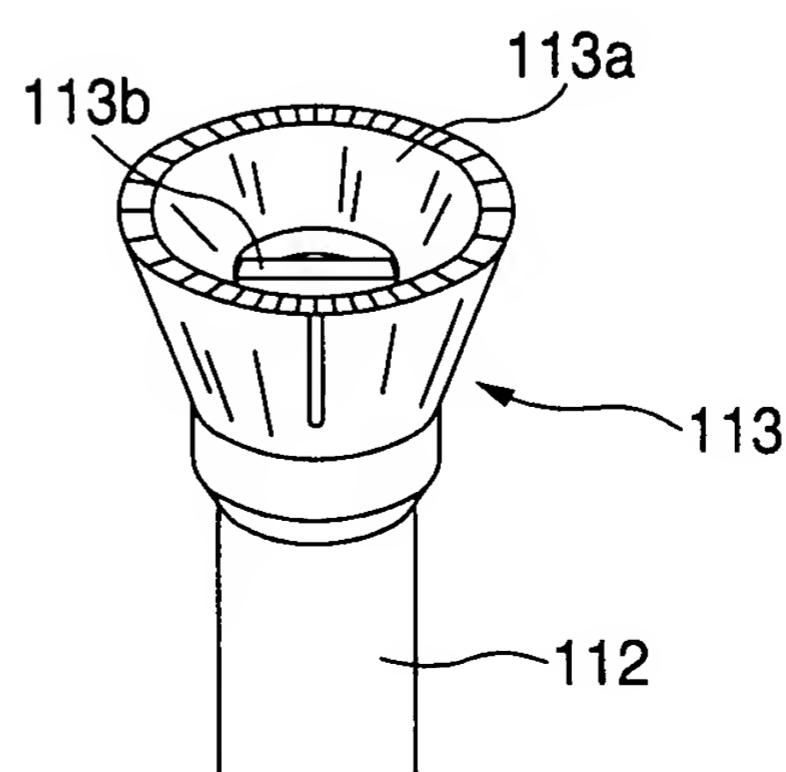

Q76299
10/603,927 Filed: 6/26/03
Darryl Mexic (202) 293-7060
Toshiaki MIZUNO, et al.
**DRAINING DEVICE AND LENS PROCESSING
SYSTEM HAVING THE SAME**
Page 5 of 9

FIG. 6


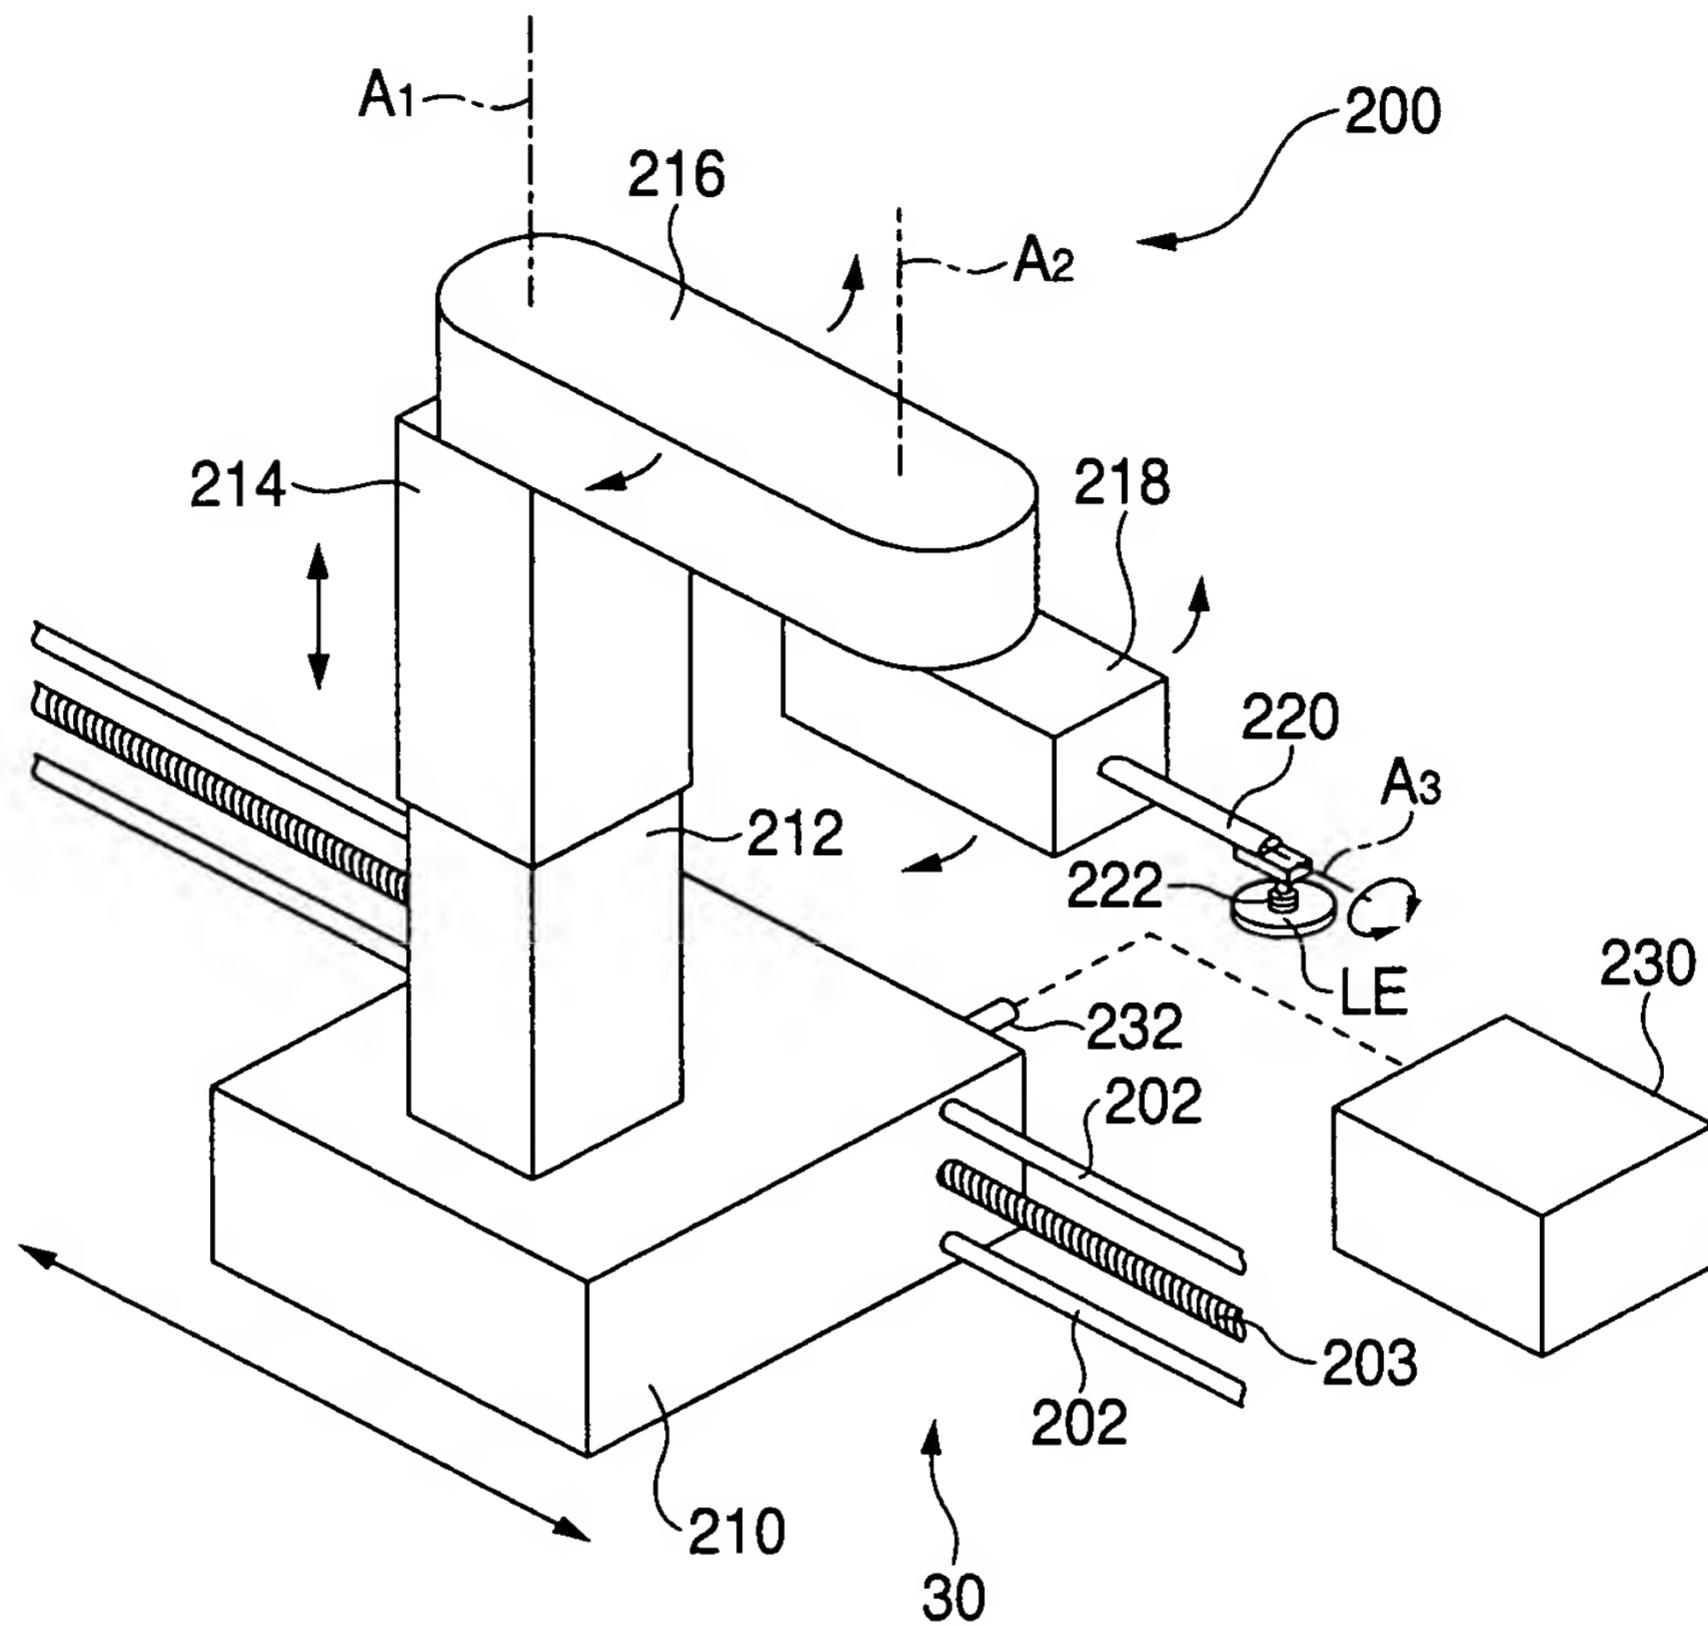



FIG. 7



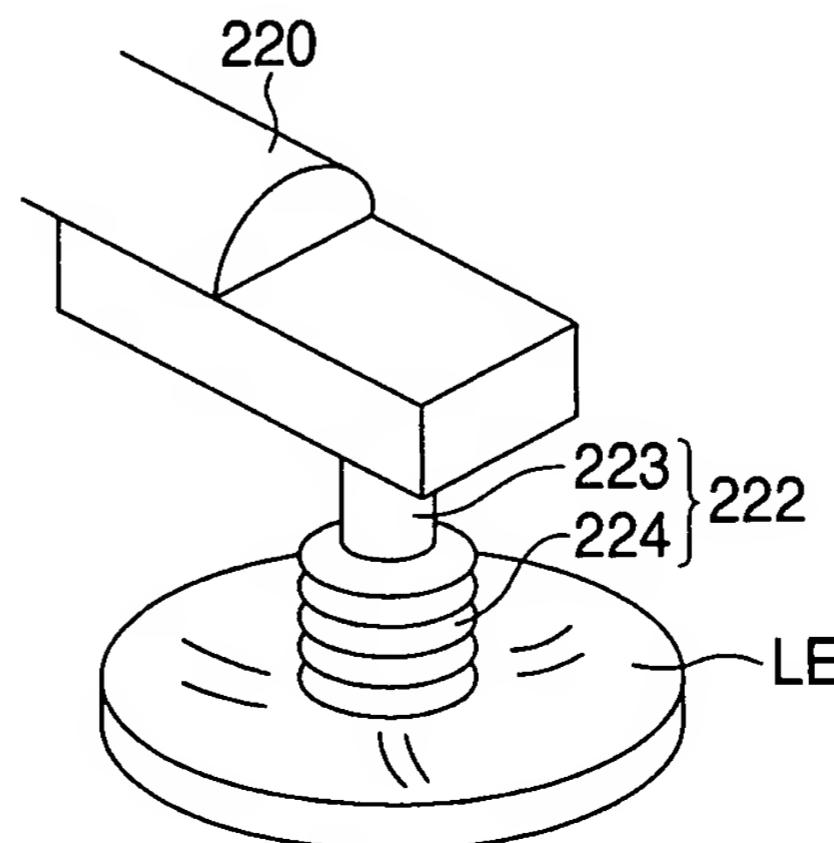

Q76299
10/603,927 Filed: 6/26/03
Darryl Mexic (202) 293-7060
Toshiaki MIZUNO, et al.
DRAINING DEVICE AND LENS PROCESSING
SYSTEM HAVING THE SAME
Page 6 of 9


FIG. 8

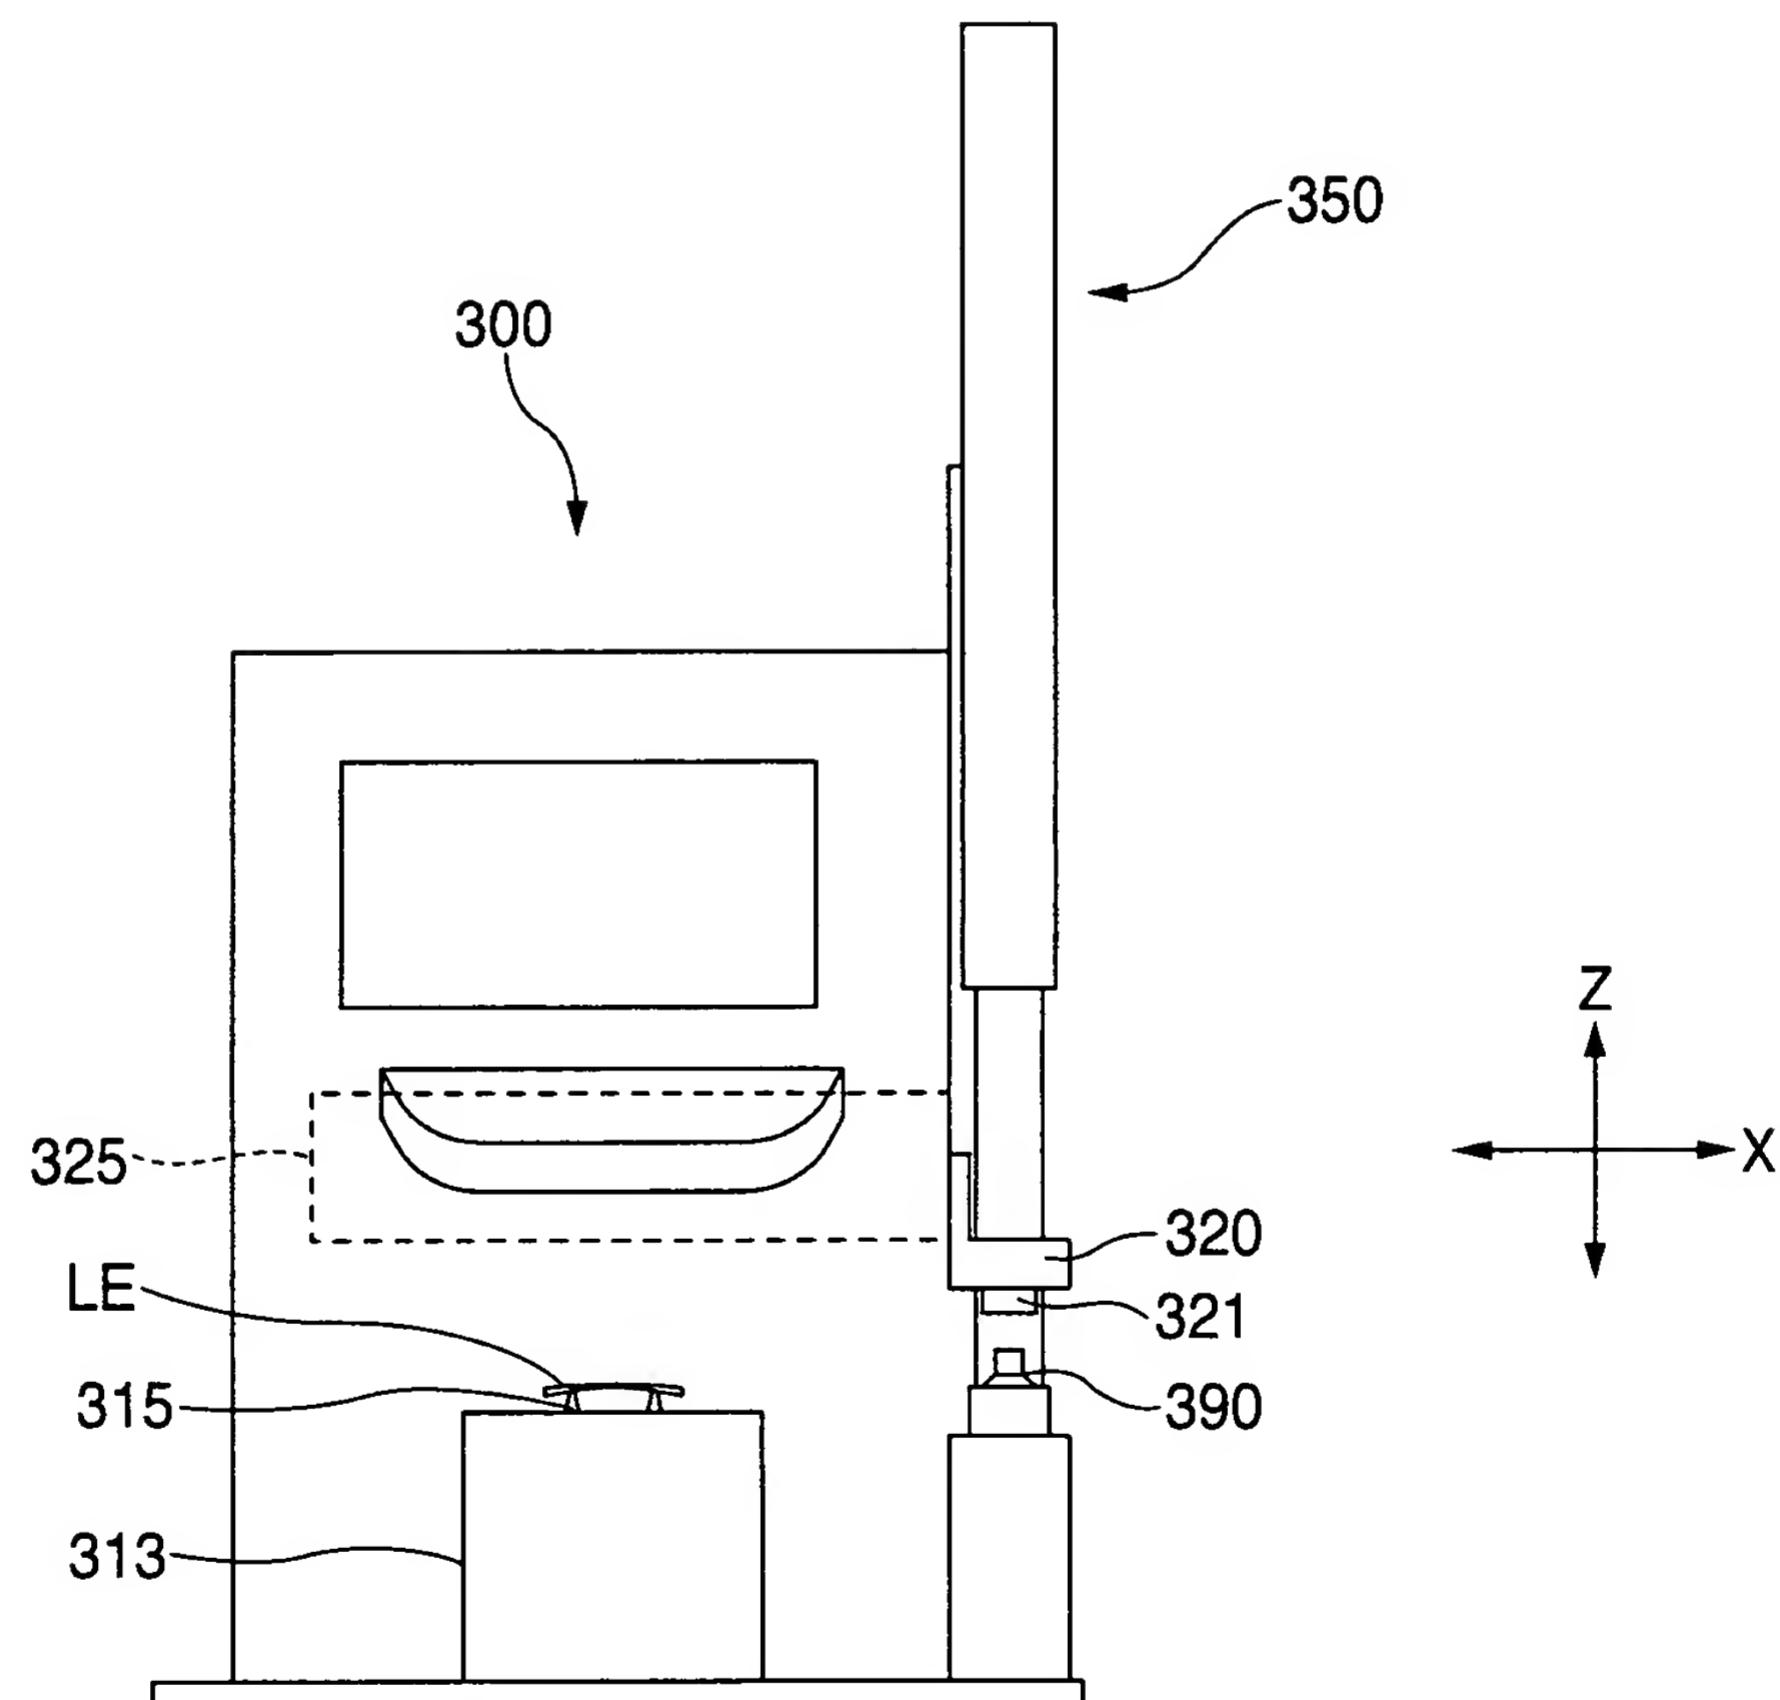



Q76299
10/603,927 Filed: 6/26/03
Darryl Mexic (202) 293-7060
Toshiaki MIZUNO, et al.
DRAINING DEVICE AND LENS PROCESSING
SYSTEM HAVING THE SAME
Page 7 of 9

FIG. 9

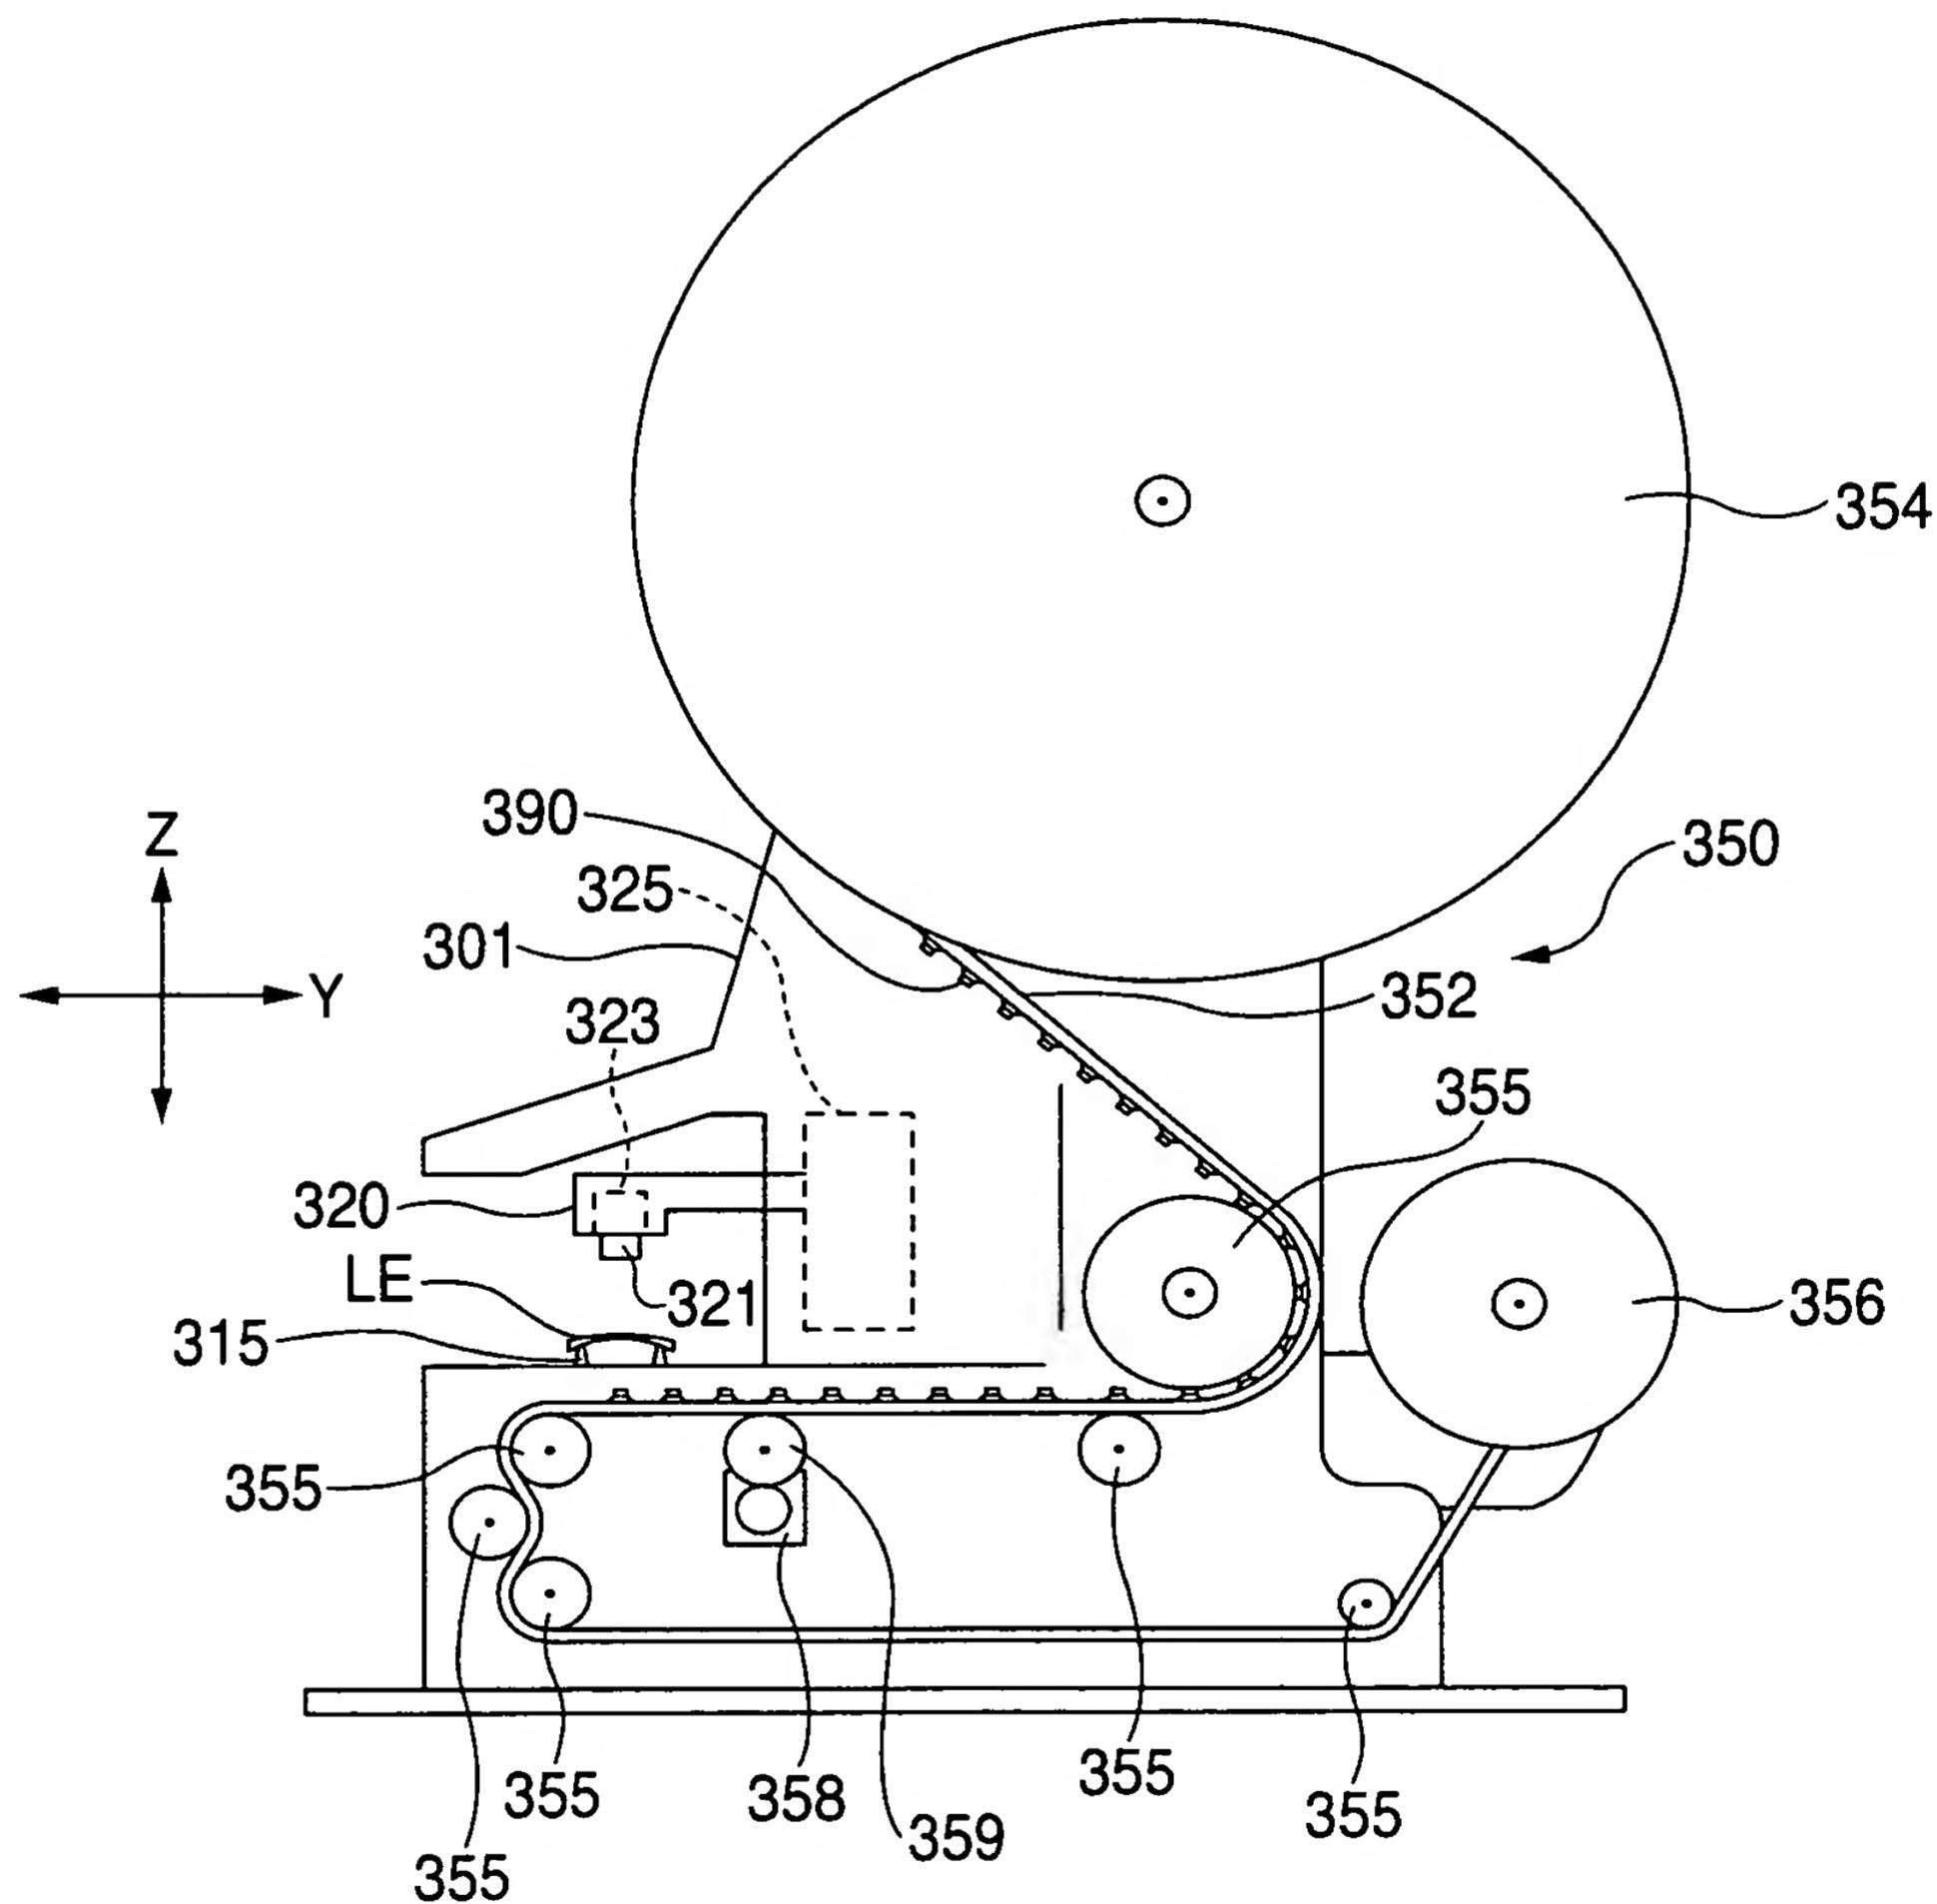



Q76299
10/603,927 Filed: 6/26/03
Darryl Mexic (202) 293-7060
Toshiaki MIZUNO, et al.
DRAINING DEVICE AND LENS PROCESSING
SYSTEM HAVING THE SAME
Page 8 of 9

FIG. 10


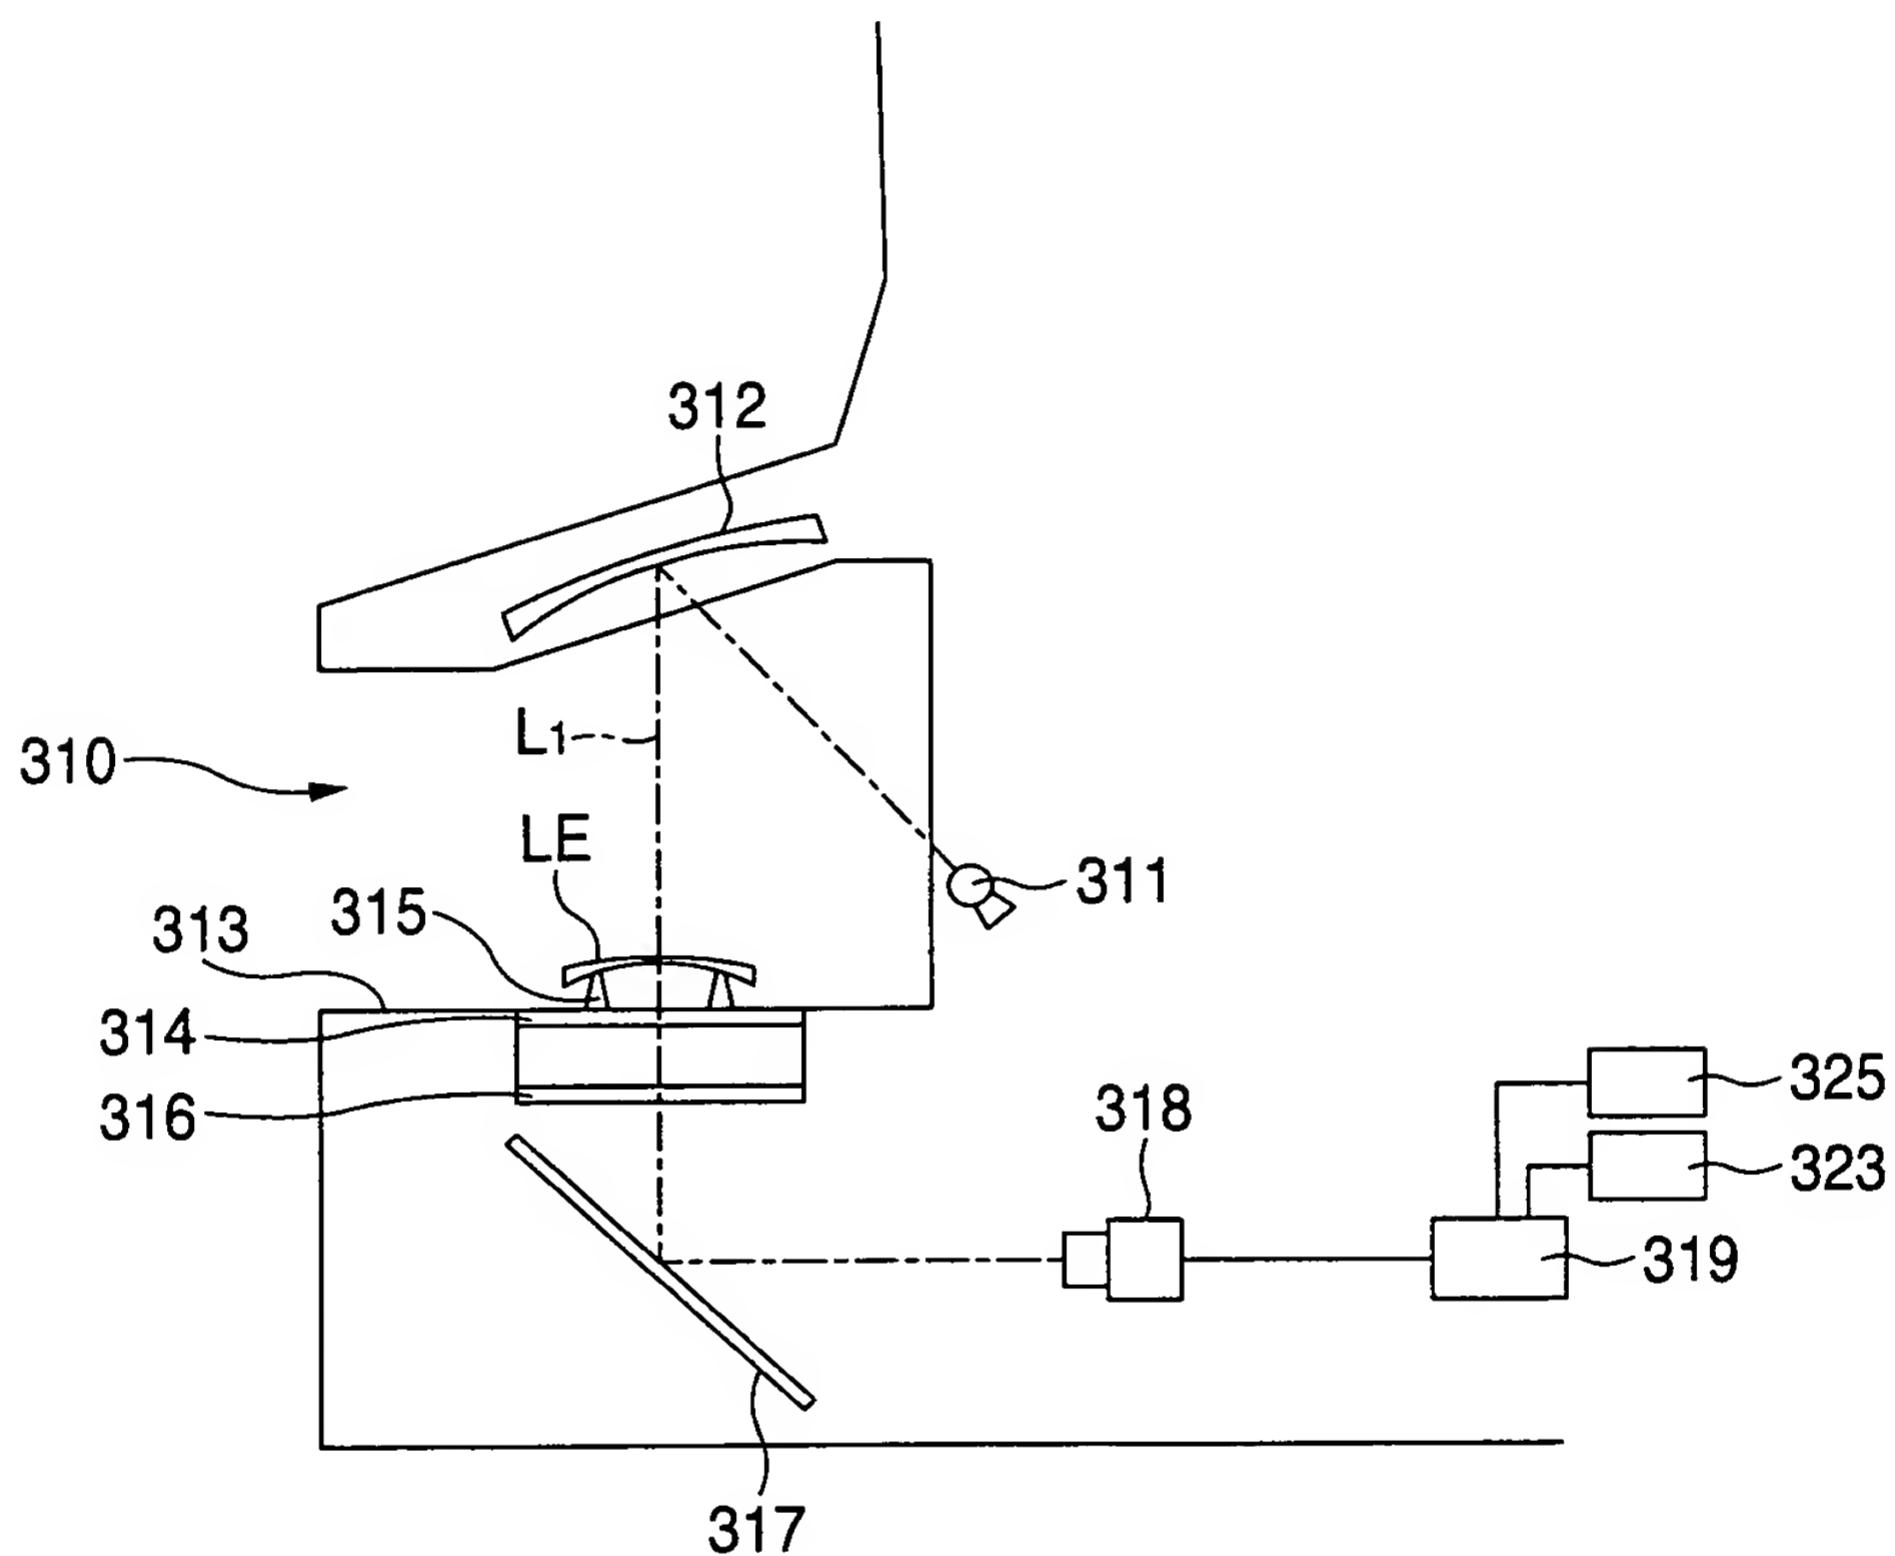


FIG. 11



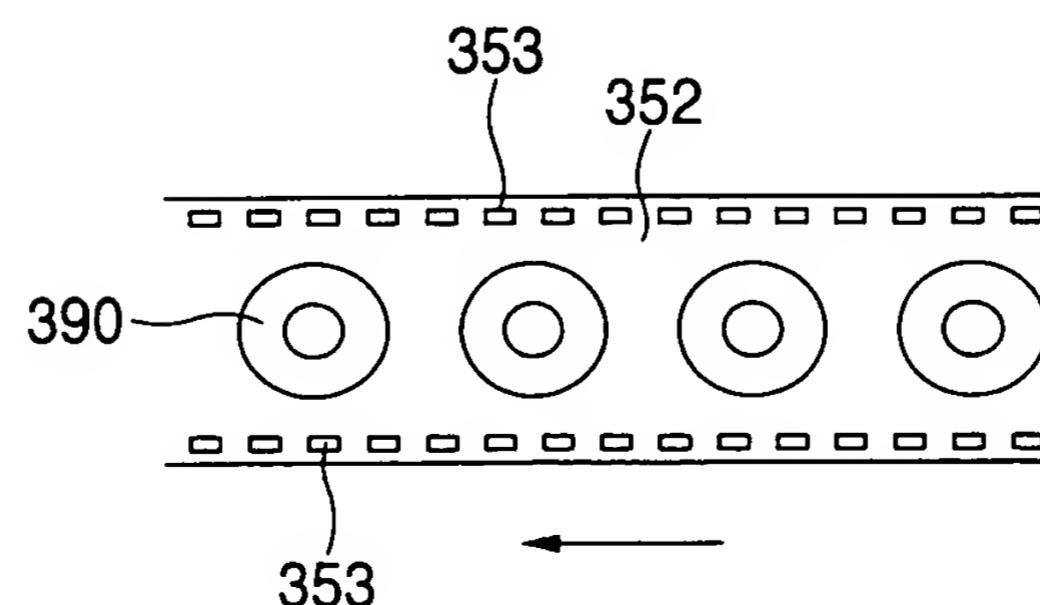

Q76299
10/603,927 Filed: 6/26/03
Darryl Mexic (202) 293-7060
Toshiaki MIZUNO, et al.
DRAINING DEVICE AND LENS PROCESSING
SYSTEM HAVING THE SAME
Page 9 of 9

FIG. 12

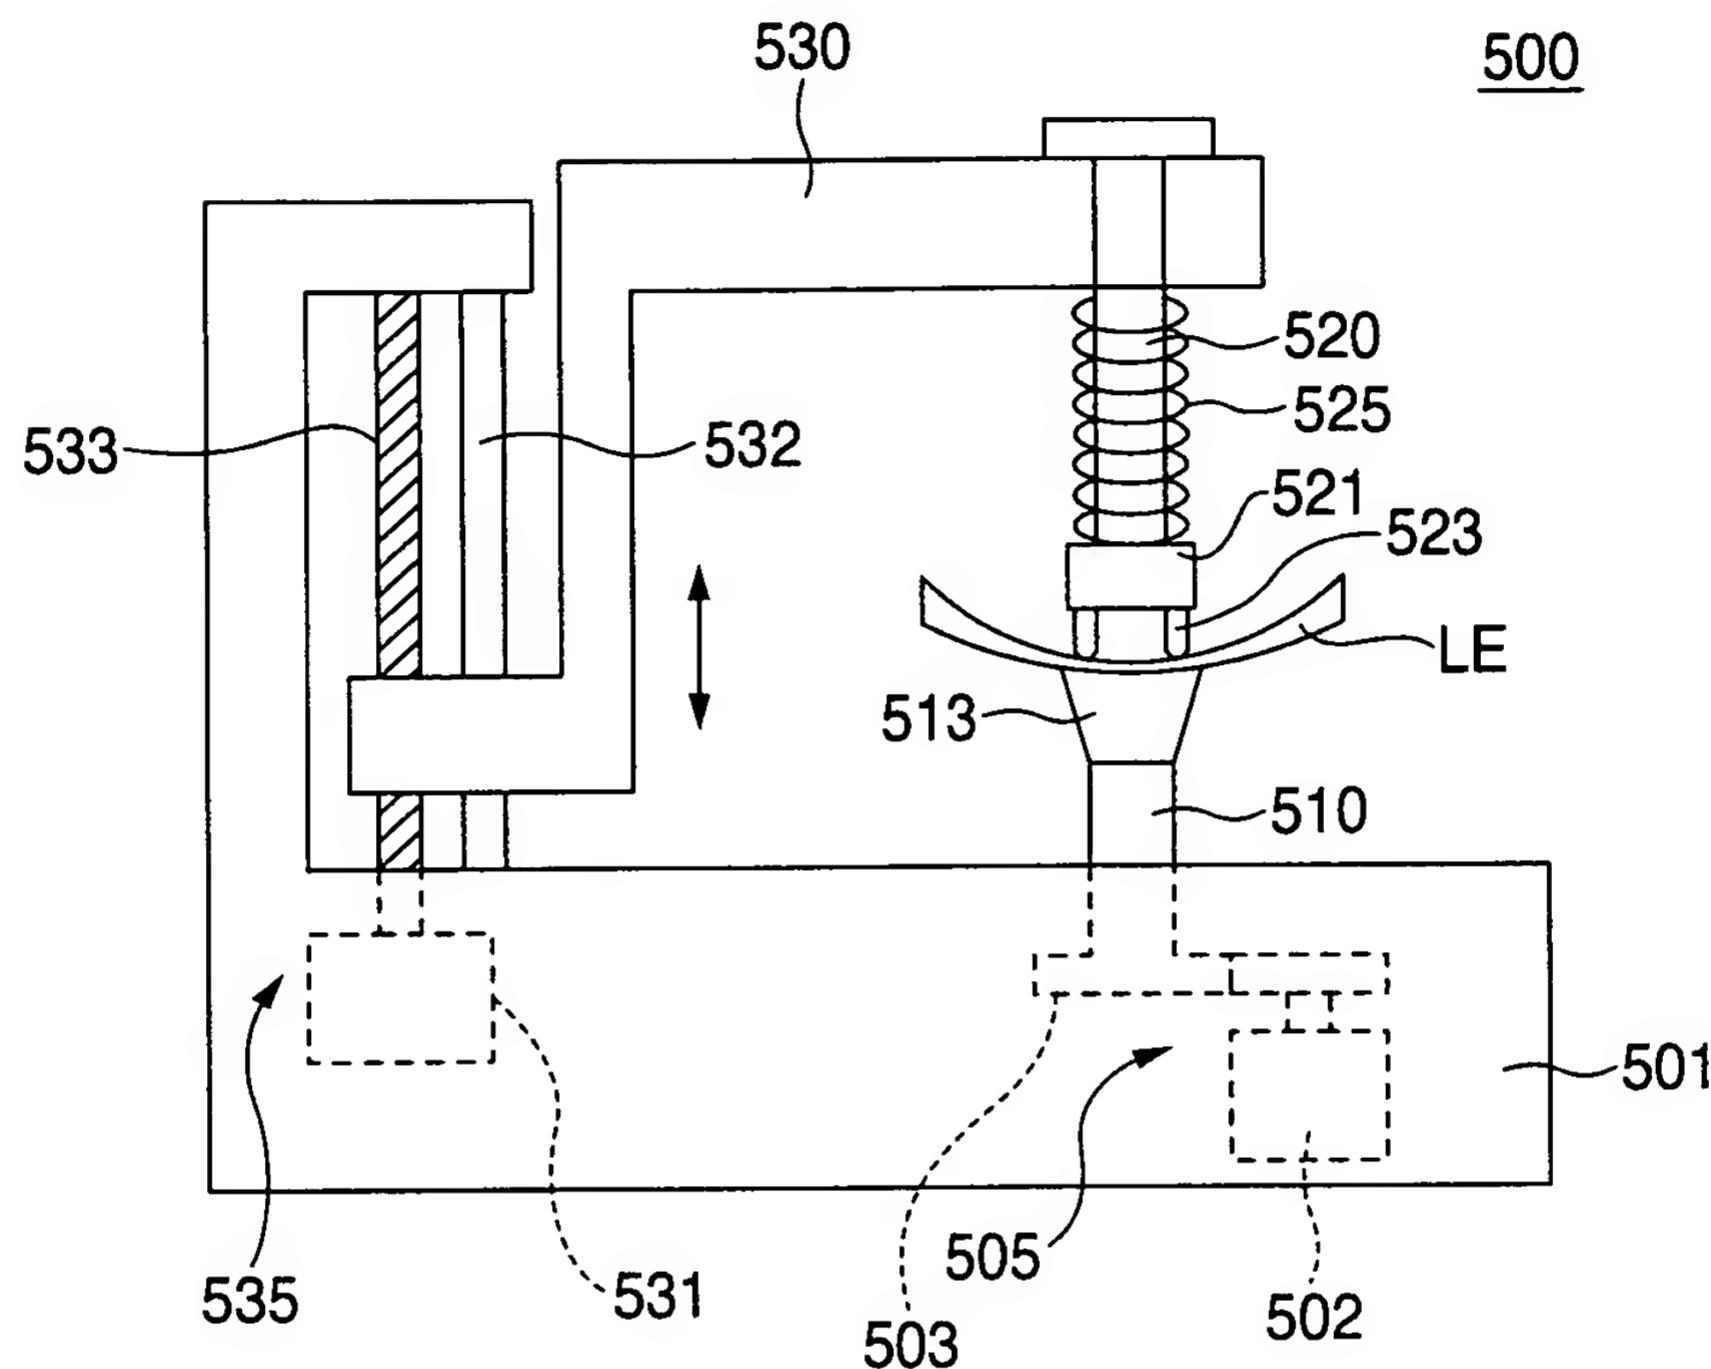


FIG. 13

